# TenaTac®

## Instructions for correct application
## Robot-assisted laparoscopic surgery

FRM751-118
Rev. 00 2025-07

### General steps

**Step 1:** Ensure that gloves, instruments and the inside of the trocar are clean and dry

**Step 2:** Take TenaTac® from the packaging using sterile technique

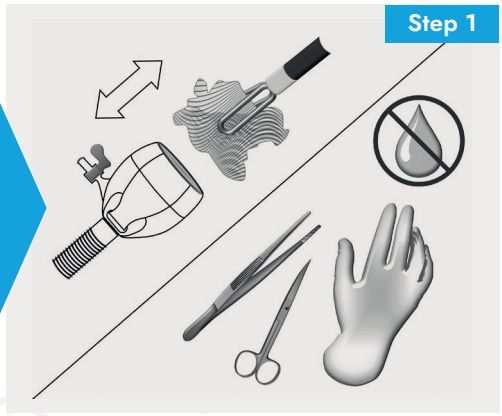


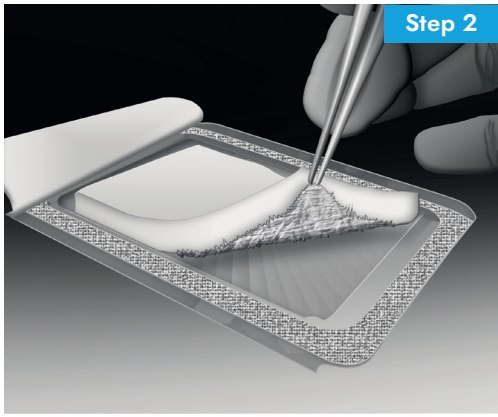


**Step 3:** Cut TenaTac® to size if required

**Step 4:** Compress TenaTac® to enhance flexibility for easier application

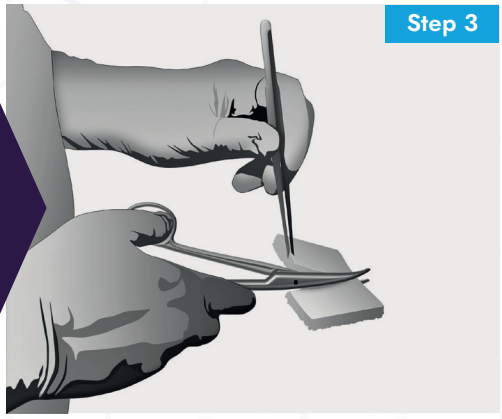


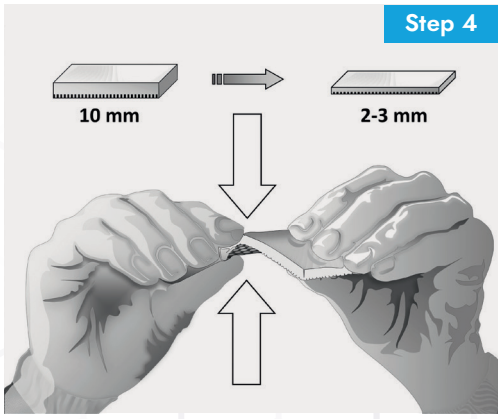


**Step 5:** Fold Tenatac® inwards, columns outside

**Step 6:** Insert TenaTac® through the trocar, grasping distal end

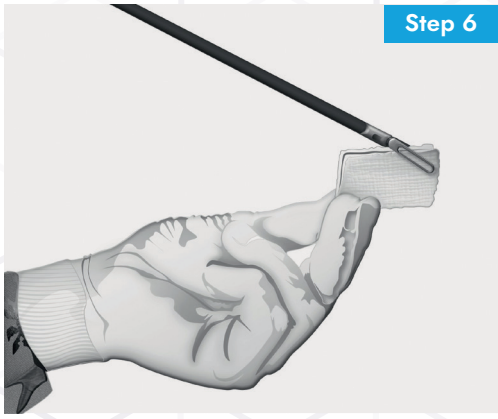


**Step 7:** Unfold TenaTac® with columns on tissue and/or staple line. Dab with a wet compress using light pressure for 2-3 minutes. Add saline to the gauze instead of directly on patch.

**Step 8:** Make sure that TenaTac® turns into a transparent adhesive gel that is sufficiently flexible and elastic to adapt to the structure and movements of the organs

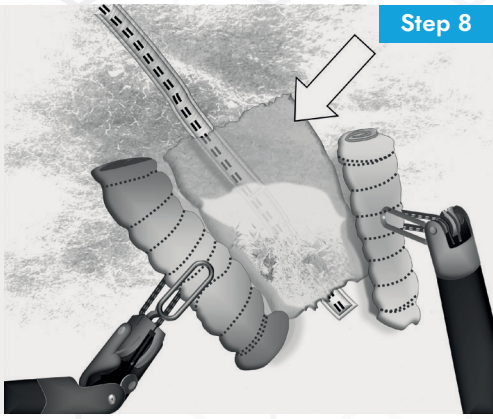


**Primary Distributor**
CuraMedrix B.V.
The Netherlands

**Enquiries contact**
r.van.beek@curamedrix.com
or sales@curamedrix.com

*TenaTac® is a registered trademark of Selentus Science Ltd.*

SCAN QR-CODE TO VIEW THE 'HOW TO USE' VIDEO ON YOUTUBE